



**Rapid Thyrotropin (Rapid TSH)
Test System
Product Code: 6025-300**

1.0 INTRODUCTION

Intended Use: The Quantitative Determination of Thyroid Stimulating Hormone or Thyrotropin (TSH) Concentration in Human Serum by a Microplate Enzyme Immunoassay, Colorimetric

2.0 SUMMARY AND EXPLANATION OF THE TEST

Measurement of the serum concentration of thyrotropin (TSH), a glycoprotein with a molecular weight of 28,000 daltons and secreted from the anterior pituitary, is generally regarded as the most sensitive indicator available for the diagnosis of primary and secondary (pituitary) hypothyroidism.^{1,2} Increase in serum concentrations of TSH, which is primarily responsible for the synthesis and release of thyroid hormones, is an early and sensitive indicator of decrease thyroid reserve and in conjunction with decreased thyroxine (T4) concentrations is diagnostic of primary hypothyroidism. The expected increase in TSH concentrations demonstrates the classical negative feedback system between the pituitary and thyroid glands; that is, primary thyroid gland failure reduces secretion of the thyroid hormones, which in turn stimulates the release of TSH from the pituitary.

Additionally, TSH measurements are equally useful in differentiating secondary and tertiary (hypothalamic) hypothyroidism from the primary thyroid disease. TSH release from the pituitary is regulated by thyrotropin releasing factor (TRH), which is secreted by the hypothalamus, and by direct action of T4 and triiodothyronine (T3), the thyroid hormones, at the pituitary. Increased levels of T3 and T4 reduce the response of the pituitary to the stimulatory effects of TRH. In secondary and tertiary hypothyroidism, concentrations of T4 are usually low and TSH levels are generally low or normal. Either pituitary TSH deficiency (secondary hypothyroidism) or insufficiency of stimulation of the pituitary by TRH (tertiary hypothyroidism) causes this. The TRH stimulation test differentiates these conditions. In secondary hypothyroidism, TSH response to TRH is blunted while a normal or delayed response is obtained in tertiary hypothyroidism.

Further, the advent of immunoenzymometric assays has provided the laboratory with sufficient sensitivity to enable the differentiating of hyperthyroidism from euthyroid population and extending the usefulness of TSH measurements. This method is a second-generation assay, which provides the means for discrimination in the hyperthyroid-euthyroid range. The functional sensitivity (<20% between assay CV) of the one-hour procedure is 0.195 µIU/ml while the two-hour procedure has a functional sensitivity of 0.095µIU/ml.³

In this method, TSH calibrator, patient specimen or control is first added to a streptavidin coated well. Biotinylated monoclonal and enzyme labeled antibodies are added and the reactants mixed. Reaction between the various TSH antibodies and native TSH

forms a sandwich complex that binds with the streptavidin coated to the well.

After the completion of the required incubation period, the antibody bound enzyme-thyrotropin conjugate is separated from the unbound enzyme-thyrotropin conjugate by aspiration or decantation. The activity of the enzyme present on the surface of the well is quantitated by reaction with a suitable substrate to produce color.


The employment of several serum references of known thyrotropin levels permits construction of a dose response curve of activity and concentration. From comparison to the dose response curve, an unknown specimen's activity can be correlated with thyrotropin concentration.

3.0 PRINCIPLE

Immunoenzymometric assay (TYPE 3):


The essential reagents required for an immunoenzymometric assay include high affinity and specificity antibodies (enzyme conjugated and immobilized), with different and distinct epitope recognition, **in excess**, and native antigen. In this procedure, the immobilization takes place during the assay at the surface of a microplate well through the interaction of streptavidin coated on the well and exogenously added biotinylated monoclonal anti-TSH antibody.

Upon mixing monoclonal biotinylated antibody, the enzyme-labeled antibody and a serum containing the native antigen, reaction results between the native antigen and the antibodies, without competition or steric hindrance, to form a soluble sandwich complex. The interaction is illustrated by the following equation:



${}^{Bn}Ab_{(m)}$ = Biotinylated Monoclonal Antibody (Excess Quantity)
 Ag_{TSH} = Native Antigen (Variable Quantity)
 ${}^{Enz}Ab_{(p)}$ = Enzyme - Polyclonal Antibody (Excess Quantity)
 ${}^{Enz}Ab_{(p)} - Ag_{TSH} - {}^{Bn}Ab_{(m)}$ = Antigen-Antibodies Sandwich Complex
 k_a = Rate Constant of Association
 k_{-a} = Rate Constant of Dissociation

Simultaneously, the complex is deposited to the well through the high affinity reaction of streptavidin and biotinylated antibody. This interaction is illustrated below:



After equilibrium is attained, the antibody bound fraction is separated from unbound antigen by decantation or aspiration. The enzyme activity in the antibody bound fraction is directly proportional to the native antigen concentration. By utilizing several different serum references of known antigen values, a dose response curve can be generated from which the antigen concentration of an unknown can be ascertained.

4.0 REAGENTS

Materials Provided:

- A. Rapid TSH Calibrators – 1ml/vial - Icons A-F**
Six (6) vials of references for TSH Antigen at levels of 0(A), 0.5(B), 2.5(C), 10.0(D), 30(E) and 100(F) µIU/ml. A preservative has been added. Store at 2-8°C.
Note: The calibrators, human serum based, were calibrated using a reference preparation, which was assayed against the WHO 2nd IRP 80/558.
- B. Rapid TSH Enzyme Reagent – 13ml/vial - Icon**
One (1) vial contains enzyme labeled affinity purified polyclonal goat antibody, biotinylated monoclonal mouse IgG in buffer, dye, and preservative. Store at 2-8°C.
- C. Streptavidin Coated Plate – 96 wells – Icon**
One 96-well microplate coated with streptavidin and packaged in an aluminum bag with a drying agent. Store at 2-8°C.
- D. Wash Solution Concentrate – 20ml/vial - Icon**
One (1) vial contains a surfactant in buffered saline. A preservative has been added. Store at 2-8°C.

- E. Substrate A – 7ml/vial - Icon**
One (1) vial contains tetramethylbenzidine (TMB) in buffer. Store at 2-8°C. See “Reagent Preparation.”
- F. Substrate B – 7ml/vial - Icon**
One (1) vial contains hydrogen peroxide (H₂O₂) in buffer. Store at 2-8°C. See “Reagent Preparation.”
- G. Stop Solution – 8ml/vial - Icon**
One (1) vial contains a strong acid (1N HCl). Store at 2-8°C.
- H. Product Instructions.**

- Note 1:** Do not use reagents beyond the kit expiration date.
- Note 2:** Avoid extended exposure to heat and light. **Opened reagents are stable for sixty (60) days when stored at 2-8°C. Kit and component stability are identified on the label.**
- Note 3:** Above reagents are for a single 96-well microplate.

4.1 Materials Required But Not Provided:

1. Pipette(s) capable of delivering 0.025 & 0.050ml (25 & 50µl) volumes with a precision of better than 1.5%.
2. Dispenser(s) for repetitive deliveries of 0.100 & 0.350ml (100 & 350µl) volumes with a precision of better than 1.5%.
3. Microplate washer or a squeeze bottle (optional).
4. Microplate Reader with 450nm and 620nm wavelength absorbance capability.
5. Absorbent Paper for blotting the microplate wells.
6. Plastic wrap or microplate cover for incubation steps.
7. Vacuum aspirator (optional) for wash steps.
8. Timer.
9. Storage container for storage of wash buffer.
10. Distilled or deionized water.
11. Quality Control Materials.

5.0 PRECAUTIONS

**For In Vitro Diagnostic Use
Not for Internal or External Use in Humans or Animals**

All products that contain human serum have been found to be non-reactive for Hepatitis B Surface antigen, HIV 1&2 and HCV antibodies by FDA required tests. Since no known test can offer complete assurance that infectious agents are absent, all human serum products should be handled as potentially hazardous and capable of transmitting disease. Good laboratory procedures for handling blood products can be found in the Center for Disease Control / National Institute of Health, "Biosafety in Microbiological and Biomedical Laboratories," 2nd Edition, 1988, HHS

Safe disposal of kit components must be according to local regulatory and statutory requirement.

6.0 SPECIMEN COLLECTION AND PREPARATION

The specimens shall be blood serum and the usual precautions in the collection of venipuncture samples should be observed. For accurate comparison to established normal values, a fasting morning serum sample should be obtained. The blood should be collected in a plain redtop venipuncture tube without additives or gel barrier. Allow the blood to clot. Centrifuge the specimen to separate the serum from the cells.

In patients receiving therapy with high biotin doses (i.e. >5mg/day), no sample should be taken until at least 8 hours after the last biotin administration, preferably overnight to ensure fasting sample.

Samples may be refrigerated at 2-8°C for a maximum period of five (5) days. If the specimen(s) cannot be assayed within this time, the sample(s) may be stored at temperatures of -20°C for up to 30 days. Avoid use of contaminated devices. Avoid repetitive freezing and thawing. When assayed in duplicate, 0.050ml (50µl) of the specimen is required.

7.0 QUALITY CONTROL

Each laboratory should assay controls at levels in the low, normal, and elevated range for monitoring assay performance. These controls should be treated as unknowns and values determined in every test procedure performed. Quality control charts should be maintained to follow the performance of the supplied reagents. Pertinent statistical methods should be employed to ascertain

trends. The individual laboratory should set acceptable assay performance limits. Other parameters that should be monitored include the 80, 50 and 20% intercepts of the dose response curve for run-to-run reproducibility. In addition, maximum absorbance should be consistent with past experience. Significant deviation from established performance can indicate unnoticed change in experimental conditions or degradation of kit reagents. Fresh reagents should be used to determine the reason for the variations.

8.0 REAGENT PREPARATION

- 1. Wash Buffer**
Dilute contents of wash concentrate to 1000ml with distilled or deionized water in a suitable storage container. The diluted buffer can be stored at 2-30°C for up to 60 days.
- 2. Working Substrate Solution – Stable for one (1) year.**
Pour the contents of the amber vial labeled Solution 'A' into the clear vial labeled Solution 'B'. Place the yellow cap on the clear vial for easy identification. Mix and label accordingly. Store at 2 - 8°C.

Note 1: Do not use the working substrate if it looks blue.
Note 2: Do not use reagents that are contaminated or have bacteria growth.

9.0 TEST PROCEDURE

*Before proceeding with the assay, bring all reagents, reference calibrators and controls to room temperature (20 - 27° C).
****Test Procedure should be performed by a skilled individual or trained professional*****

1. Format the microplates' wells for each serum reference calibrator, control and patient specimen to be assayed in duplicate. **Replace any unused microwell strips back into the aluminum bag, seal and store at 2-8°C.**
2. Pipette 0.025ml (25µl) of the appropriate serum reference calibrator, control or specimen into the assigned well.
3. Add 0.100ml (100µl) of the Rapid TSH Enzyme Reagent to each well. **It is very important to dispense all reagents close to the bottom of the coated well.**
4. Swirl the microplate gently for 20-30 seconds to mix and cover.
5. Incubate 30 minutes at room temperature.
6. Discard the contents of the microplate by decantation or aspiration. If decanting, tap and blot the plate dry with absorbent paper.
7. Add 0.350ml (350µl) of wash buffer (see Reagent Preparation Section) decant (tap and blot) or aspirate. Repeat two (2) additional times for a total of three (3) washes. **An automatic or manual plate washer can be used. Follow the manufacturer's instruction for proper usage. If a squeeze bottle is employed, fill each well by depressing the container (avoiding air bubbles) to dispense the wash. Decant the wash and repeat two (2) additional times.**
8. Add 0.100ml (100µl) of working substrate solution to all wells (see Reagent Preparation Section). **Always add reagents in the same order to minimize reaction time differences between wells.**
- DO NOT SHAKE THE PLATE AFTER SUBSTRATE ADDITION**
9. Incubate at room temperature for fifteen (15) minutes.
10. Add 0.050ml (50µl) of stop solution to each well and mix gently for 15-20 seconds. **Always add reagents in the same order to minimize reaction time differences between wells.**
11. Read the absorbance in each well at 450nm (using a reference wavelength of 620-630nm to minimize well imperfections) in a microplate reader. **The results should be read within thirty (30) minutes of adding the stop solution.**

**** For better low-end sensitivity (< 0.5µIU/ml), incubate 60 minutes at room temperature. The 100µIU/ml calibrator should be excluded since absorbance over 3.0 units will be experienced. Follow the remaining steps.**

Note 1: Dilute samples reading over 100 µIU/ml by 1:5 and 1:10 with TSH '0' Calibrator. Multiply the results by the dilution factor to obtain accurate results.
Note 2: If additional diluting matrix is needed, a universal serum diluent can be purchased by calling your representative or Monobind directly.

10.0 CALCULATION OF RESULTS


A dose response curve is used to ascertain the concentration of thyrotropin in unknown specimens.

1. Record the absorbance obtained from the printout of the microplate reader as outlined in Example 1
2. Plot the absorbance for each duplicate serum reference versus the corresponding TSH concentration (in $\mu\text{IU/ml}$) on linear graph paper (do not average the duplicates of the serum references before plotting).
3. Draw the best-fit curve through the plotted points.
4. To determine the concentration of TSH for an unknown, locate the average absorbance of the duplicates for each unknown on the vertical axis of the graph, find the intersecting point on the curve, and read the concentration (in $\mu\text{IU/ml}$) from the horizontal axis of the graph (the duplicates of the unknown may be averaged as indicated). In the following example, the average absorbance 1.227 intersects the dose response curve at 35.0 $\mu\text{IU/ml}$ TSH concentration (See Figure 1).

EXAMPLE 1

Sample I.D.	Well Number	Abs	Mean Abs	Value ($\mu\text{IU/ml}$)
Cal A	A1	0.007	0.019	0
	B1	0.009		
Cal B	C1	0.023	0.022	0.5
	D1	0.020		
Cal C	E1	0.104	0.108	2.5
	F1	0.112		
Cal D	G1	0.397	0.387	10
	H1	0.377		
Cal E	A2	1.101	1.098	30
	B2	1.095		
Cal F	C2	2.600	2.570	100
	D2	2.540		
Control	G2	0.026	0.027	0.524
	H2	0.028		
Patient	A3	1.227	1.227	35.0
	B3	1.227		

Figure 1

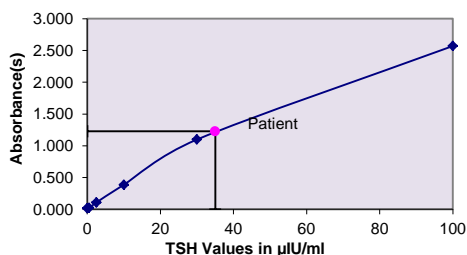

*The data presented in Example 1 and Figure 1 are for illustration only and **should not** be used in lieu of a dose response curve prepared with each assay.

11.0 Q.C. PARAMETERS

In order for the assay results to be considered valid the following criteria should be met:

1. The absorbance of calibrator 'F' (100 $\mu\text{IU/ml}$) should be ≥ 1.3 .
2. Four out of six quality control pools should be within the established ranges.

12.0 RISK ANALYSIS

The MSDS and Risk Analysis Form for this product are available on request from Monobind Inc.

12.1 Assay Performance

1. It is important that the time of reaction in each well is held constant to achieve reproducible results.
2. Pipetting of samples should not extend beyond ten (10) minutes to avoid assay drift.
3. Highly lipemic, hemolyzed or grossly contaminated specimen(s) should not be used.
4. If more than one (1) plate is used, it is recommended to repeat the dose response curve.
5. The addition of substrate solution initiates a kinetic reaction, which is terminated by the addition of the stop solution. Therefore, the substrate and stop solution should be added in the same sequence to eliminate any time-deviation during reaction.
6. Plate readers measure vertically. Do not touch the bottom of the wells.
7. Failure to remove adhering solution adequately in the aspiration or decantation wash step(s) may result in poor replication and spurious results.
8. Use components from the same lot. No intermixing of reagents from different batches.
9. Accurate and precise pipetting, as well as following the exact time and temperature requirements prescribed are essential. Any deviation from Monobind's IFU may yield inaccurate results.
10. All applicable national standards, regulations and laws, including, but not limited to, good laboratory procedures, must be strictly followed to ensure compliance and proper device usage.
11. It is important to calibrate all the equipment e.g. Pipettes, Readers, Washers and/or the automated instruments used with this device, and to perform routine preventative maintenance.
12. Risk Analysis- as required by CE Mark IVD Directive 98/79/EC - for this and other devices, made by Monobind, can be requested via email from Monobind@monobind.com.

12.2 Interpretation

1. **Measurements and interpretation of results must be performed by a skilled individual or trained professional.**
2. Laboratory results alone are only one aspect for determining patient care and should not be the sole basis for therapy, particularly if the results conflict with other determinants.
3. The reagents for the test system procedure have been formulated to eliminate maximal interference; however, potential interaction between rare serum specimens and test reagents can cause erroneous results. Heterophilic antibodies often cause these interactions and have been known to be problems for all kinds of immunoassays. (Boscato LM Stuart MC. 'Heterophilic antibodies: a problem for all immunoassays' Clin.Chem. 1988:3427-33). For diagnostic purposes, the results from this assay should be used in combination with clinical examination, patient history and all other clinical findings.
4. For valid test results, adequate controls and other parameters must be within the listed ranges and assay requirements.
5. If test kits are altered, such as by mixing parts of different kits, which could produce false test results, or if results are incorrectly interpreted, **Monobind shall have no liability.**
6. If computer controlled data reduction is used to interpret the results of the test, it is imperative that the predicted values for the calibrators fall within 10% of the assigned concentrations.
7. Serum TSH concentration is dependent upon a multiplicity of factors: hypothalamus gland function, thyroid gland function, and the responsiveness of pituitary to TRH. Thus, thyrotropin concentration alone is not sufficient to assess clinical status.
8. Serum TSH values may be elevated by pharmacological intervention. Domperidone, amiodazon, iodide, phenobarbital, and phenytoin have been reported to increase TSH levels.
9. A decrease in thyrotropin values has been reported with the administration of propranolol, methimazol, dopamine and d-thyroxine.⁴
10. Genetic variations or degradation of intact TSH into subunits may affect the binding characteristics of the antibodies and influence the final result. Such samples normally exhibit different results among various assay systems due to the reactivity of the antibodies involved.

NOT INTENDED FOR NEWBORN SCREENING

13.0 EXPECTED RANGES OF VALUES

A study of euthyroid adult population was undertaken to determine expected values for the Rapid TSH AccuBind® ELISA Test

System. The number and determined range are given in Table 1. A nonparametric method (95% Percentile Estimate) was used.

TABLE 1 Expected Values for the Rapid TSH Test System (in $\mu\text{IU/ml}$)		
Number	139	
Low Normal Range	0.39	
High Normal Range	6.16	
70% Confidence Intervals for 2.5 Percentile		
Low Range	0.28 – 0.53	
High Range	5.60 – 6.82	

It is important to keep in mind that establishment of a range of values, which can be expected to be found by a given method for a population of "normal" persons, is dependent upon a multiplicity of factors: the specificity of the method, the population tested and the precision of the method in the hands of the analyst. For these reasons, each laboratory should depend upon the range of expected values established by the manufacturer only until an in-house range can be determined by the analysts using the method with a population indigenous to the area in which the laboratory is located.

14.0 PERFORMANCE CHARACTERISTICS

14.1 Precision

The within and between assay precisions of the Rapid TSH AccuBind® ELISA test system were determined by analyses on three different levels of pool control sera. The number (N), mean (X) value, standard deviation (σ) and coefficient of variation (C.V.) for each of these control sera are presented in Tables 2 and 3.

TABLE 2 Within Assay Precision (Values in $\mu\text{IU/ml}$)				
Sample	N	X	σ	C.V.
Pool 1	24	0.37	0.03	8.1%
Pool 2	24	6.75	0.43	6.4%
Pool 3	24	29.30	1.94	6.6%

TABLE 3 Between Assay Precision* (Values in $\mu\text{IU/ml}$)				
Sample	N	X	σ	C.V.
Pool 1	10	0.43	0.04	9.3%
Pool 2	10	6.80	0.54	7.9%
Pool 3	10	28.40	1.67	5.9%

*As measured in ten experiments in duplicate over seven days.

14.2 Sensitivity

The sensitivity of the Rapid TSH AccuBind® ELISA Test System (detection limit) was ascertained by determining the variability of the 0 $\mu\text{IU/ml}$ serum calibrator and using the 2σ (95% certainty) statistic to calculate the minimum dose. For 30 minute incubation = 0.10 $\mu\text{IU/ml}$

14.3 Accuracy

The Rapid TSH AccuBind® ELISA test system was compared with a reference method. Biological specimens from hypothyroid, euthyroid and hyperthyroid populations were used. The values ranged from 0.01 $\mu\text{IU/ml}$ – 61 $\mu\text{IU/ml}$. The total number of such specimens was 241. The least square regression equation and the correlation coefficient were computed for the Rapid TSH AccuBind® ELISA method in comparison with the reference method. The data obtained is displayed in Table 4.

TABLE 4			
Method	Mean (x)	Least Square Regression Analysis	Correlation Coefficient
Monobind	4.54	$y = 0.47 + 0.968 (x)$	0.995
Reference	4.21		

Only slight amounts of bias between the Rapid TSH AccuBind® ELISA method and the reference method are indicated by the closeness of the mean values. The least square regression equation and correlation coefficient indicates excellent method agreement.

14.4 Specificity

The cross reactivity of the Rapid TSH AccuBind® ELISA test system to selected substances was evaluated by adding the interfering substance to a serum matrix at various concentrations.

The cross-reactivity was calculated by deriving a ratio between dose of interfering substance to dose of thyrotropin needed to produce the same absorbance.

Substance	Cross Reactivity	Conc.
Thyrotropin (hTSH)	1.0000	-
Follitropin (hFSH)	< 0.0001	1000ng/ml
Lutropin Hormone (hLH)	< 0.0001	1000ng/ml
Chorionic Gonadotropin(hCG)	< 0.0001	1000ng/ml

15.0 REFERENCES

1. Hopton MR, & Harrap JJ, "Immunoradiometric assay of thyrotropin as a first line thyroid function test in the routine laboratory", *Clinical Chemistry*, 32, 691 (1986).
2. Caldwell, G et al. "A new strategy for thyroid function testing", *Lancet*, I, 1117 (1985).
3. Young DS, Pestaner LC, and Gilberman U, "Effects of Drugs on Clinical Laboratory Tests", *Clinical Chemistry*, 21, 3660 (1975).
4. Spencer, CA, et al. "Interlaboratory/Intermethod differences in Functional Sensitivity of Immunometric Assays of Thyrotropin (TSH) and Impact on Reliability of Measurement of Subnormal Concentrations of TSH", *Clinical Chemistry*, 41, 367 (1995).
5. Beck-Peccoz P, Persani L, "Variable biological activity of thyroid stimulating hormone", *Eur J Endocrinol*, 131, 331-340 (1994).
6. Bravermann, LE, "Evaluation of thyroid status in patients with thyrotoxicosis", *Clin Chem*, 42, 174-181 (1996).
7. Fisher, DA, "Physiological variations in thyroid hormones. Physiological and pathophysiological considerations", *Clin Chem*, 42, 135-139 (1996).

Revision: 3 Date: 2019-Jul-16 DCO: 1353

MP6025 Product Code: 6025-300					
Size	96(A)	192(B)	480(D)	960(E)	
Reagent (fill)	A)	1ml set	1ml set	2ml set	2ml set x2
	B)	1 (13ml)	2 (13ml)	1(60ml)	2 (60ml)
	C)	1 plate	2 plates	5 plates	10 plates
	D)	1 (20ml)	1 (20ml)	1 (60ml)	2 (60ml)
	E)	1 (7ml)	2 (7ml)	1 (30ml)	2 (30ml)
	F)	1 (7ml)	2 (7ml)	1 (30ml)	2 (30ml)
	G)	1 (8ml)	2 (8ml)	1 (30ml)	2 (30ml)

For Orders and Inquires, please contact

Monobind Inc.
100 North Pointe Drive
Lake Forest, CA 92630 USA

Tel: +1 949.951.2665 Mail: info@monobind.com
Fax: +1 949.951.3539 Fax: www.monobind.com



Please visit our website to learn more about our products and services.

Glossary of Symbols
(EN 980/ISO 15223)

IVD

In Vitro -
Diagnostic
Medical
Device



Temperature
Limitation
Storage
Condition (2-8° C)



Consult
Instructions
for Use

REF

Catalogue
Number



Contains
Sufficient
Test for Σ

LOT

Batch Code



Used By
(Expiration Day)



Date of
Manufacturer



Manufacturer

EC REP

Authorized Rep in
European Country



European
Conformity