

# Neopterin ELISA

Enzyme immunoassay for the quantitative determination  
of neopterin in human serum, plasma and urine.

**REF**      **RE59321**

      **96**

        **2-8°C**

EU: **IVD** **CE**



**I B L I N T E R N A T I O N A L G M B H**

Flughafenstrasse 52a  
D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0  
Fax: +49 (0)40-53 28 91-11

IBL@IBL-International.com  
www.IBL-International.com

## 1. INTENDED USE

Enzyme immunoassay for the quantitative determination of neopterin in human serum, plasma and urine.

## 2. SUMMARY AND EXPLANATION

Neopterin is a low molecular weight molecule belonging to the chemical group known as pteridines. It is synthesised by cellular immune reaction of macrophages and dendritic cells upon stimulation with the cytokine interferon-g and as a consequence released. Neopterin has a higher stability in body fluids which makes the sample handling and measurement easier compared to other cytokines. The low molecular weight, let neopterin molecules rapidly pass the intravascular area, where it is released in urine after glomerular filtration. The half life period in human bodies is only affected by renal excretion. So neopterin values reflect the totality of immunological processes for monocytes/macrophages and dendritic cells and can be seen as a general marker of immune activity. This characteristic feature of neopterin to reflect the different interactions of immunocompetent cells is the basis for the extraordinary status of measuring neopterin in immunological diagnosis. As a non-invasive method, urinary neopterin to creatinine ratio determination is also helpful in monitoring disease progression and the effects of therapies, as well.

Neopterin biosynthesis is closely associated with activation of the cellular immune system. Increased concentrations of neopterin were reported in patients with viral infections, suggesting that increased values may originate from the immune response of patients directed against virally infected cells. It was shown that antigenic stimulation of human peripheral blood mononuclear cells leads to neopterin release into cell culture medium and that human macrophages produce neopterin in vitro when stimulated by interferon gamma.

The determination of neopterin levels in human body fluids offers a useful and innovative tool to monitor diseases associated with the activation of cell-mediated immunity.

Increasing neopterin levels in various infections precede the clinical manifestation and seroconversion.

Normally samples are not tested for all possible infections. Therefore, the measurement of neopterin in blood donor samples is a useful tool in order to reduce the risk of infections via blood transfusion.

Other diagnostic applications for the determination of neopterin are:

- follow-up of traumatized ICU patients
- use as prognostic indication in HIV infections and malignant diseases
- early indication of complications in allograft recipients
- indication of disease activity in autoimmune diseases
- diagnosis of viral infections
- differential diagnosis of acute viral and bacterial infections
- diagnosis of tumour diseases
- follow-up control of chronic infections and monitoring of immunostimulatory therapy

## 3. TEST PRINCIPLE

Solid phase enzyme-linked immunosorbent assay (ELISA) based on the basic principle of a competitive ELISA. An unknown amount of antigen in the sample and a fixed amount of enzyme labelled antigen compete for the antibody-binding sites (rabbit-anti-neopterin). Both antigen-antibody complexes bind to the wells of the microtiter strips coated with a goat-anti-rabbit antibody. Unbound antigen is removed by washing. The intensity of the color developed after the substrate incubation is inversely proportional to the amount of antigen in the sample. Results of samples can be determined directly using the standard curve.

#### 4. WARNINGS AND PRECAUTIONS

1. For *in-vitro diagnostic* use only. For professional use only.
2. Before starting the assay, read the instructions completely and carefully. Use the valid version of the package insert provided with the kit. Be sure that everything is understood.
3. In case of severe damage of the kit package please contact IBL or your supplier in written form, latest one week after receiving the kit. Do not use damaged components in test runs, but keep safe for complaint related issues.
4. Obey lot number and expiry date. Do not mix reagents of different lots. Do not use expired reagents.
5. Follow good laboratory practice and safety guidelines. Wear lab coats, disposable latex gloves and protective glasses where necessary.
6. Reagents of this kit containing hazardous material may cause eye and skin irritations. See MATERIALS SUPPLIED and labels for details. Material Safety Data Sheets for this product are available on the IBL-Homepage or upon request directly from IBL.
7. Chemicals and prepared or used reagents have to be treated as hazardous waste according to national biohazard and safety guidelines or regulations.
8. The cleaning staff should be guided by the professionals regarding potential hazards and handling.
9. Avoid contact with Stop solution. It may cause skin irritations and burns.
10. All reagents of this kit containing human serum or plasma have been tested and were found negative for anti-HIV I/II, HBsAg and anti-HCV. However, a presence of these or other infectious agents cannot be excluded absolutely. For this reason reagents should be treated as potential biohazards in use and for disposal.

#### 5. STORAGE AND STABILITY

The kit is shipped at ambient temperature and should be stored at 2-8 °C. Keep away from heat or direct sunlight. The storage and stability of specimens and prepared reagents is stated in the corresponding chapters.

The microtiter strips are stable up to the indicated expiry after the kit is opened. Make sure that the opened bag is tightly closed when stored at 2-8 °C.

#### 6. SPECIMEN COLLECTION AND STORAGE

##### Serum, Plasma (EDTA)

The usual precautions for venipuncture should be observed. It is important to preserve the chemical integrity of a blood specimen from the moment it is collected until it is assayed. Do not use grossly hemolytic, icteric or grossly lipemic specimens. Do not use specimens containing NaN<sub>3</sub>. Samples appearing turbid should be centrifuged before testing to remove any particulate material.

Storage:	2-8 °C	≤ -20 °C (Aliquots)	Keep away from heat or direct sunlight. Avoid repeated freeze-thaw cycles.
Stability:	72 h	6 months	

##### Urine

It is possible to use spontaneous as well as 24 h urine. The total volume of urine excreted during a 24 h period should be collected and mixed in a single bottle. Preservation is not necessary. Determine total volume for calculation of results. **Mix and centrifuge samples before use in the assay.**

Storage:	2-8 °C	≤ -20 °C (Aliquots)	Keep away from heat or direct sunlight. Avoid repeated freeze-thaw cycles.
Stability:	72 h	6 months	

**7. MATERIALS SUPPLIED**

Quantity	Symbol	Component
1 x 12 x 8	<b>MTP</b>	<b>Microtiter plate</b> Break apart strips. Coated with anti-rabbit IgG (goat, polyclonal).
1 x 8 mL	<b>ANTISERUM</b>	<b>Neopterin Antiserum</b> Ready to use. Contains: Antiserum (rabbit), phosphate buffer, stabilizers.
1 x 13 mL	<b>ENZCONJ</b>	<b>Enzyme Conjugate</b> Ready to use. Contains: Neopterin, conjugated to peroxidase, phosphate buffer, stabilizers. <b>Store protected from light.</b>
1 x 6 x 1.5 mL	<b>CAL A-F</b>	<b>Standard A-F</b> 0; 1.35; 4.0; 12.0; 37.0; 111 nmol/L Ready to use. Contains: Neopterin, phosphate buffer, stabilizers.
1 x 2 x 1.5 mL	<b>CONTROL 1+2</b>	<b>Control 1+2</b> Ready to use. Concentrations / acceptable ranges see QC certificate.
1 x 21 mL	<b>ASSAYBUF</b>	<b>Assay Buffer</b> Ready to use. Contains: phosphate buffer, BSA, stabilizers.
1 x 50 mL	<b>WASHBUF CONC</b>	<b>Wash Buffer Concentrate (20x)</b> Contains: Tween, stabilizers.
1 x 19 mL	<b>TMB SUBS</b>	<b>TMB Substrate Solution</b> Contains: TMB, Buffer, stabilizers.
1 x 19 mL	<b>TMB STOP</b>	<b>TMB Stop Solution</b> Ready to use. 1 M H <sub>2</sub> SO <sub>4</sub> .
1 x	<b>FOIL</b>	<b>Adhesive Foil</b>

**8. MATERIALS REQUIRED BUT NOT SUPPLIED**

1. Micropipettes (Multipette Eppendorf or similar devices, < 3 % CV). Volume: 10; 50; 100; 1000 µL
2. Vortex mixer
3. Orbital shaker (500 rpm)
4. 8-Channel Micropipettor with reagent reservoirs
5. Additional Assay Buffer for urine dilution (can be ordered separately from IBL under **REF** KENO751).
6. Wash bottle, automated or semi-automated microtiter plate washing system
7. Microtiter plate reader capable of reading absorbance at 450 nm (reference wavelength 600-650 nm)
8. Bidistilled or deionised water
9. Paper towels, pipette tips and timer


**9. PROCEDURE NOTES**

1. Any improper handling of samples or modification of the test procedure may influence the results. The indicated pipetting volumes, incubation times, temperatures and pretreatment steps have to be performed strictly according to the instructions. Use calibrated pipettes and devices only.
2. Once the test has been started, all steps should be completed without interruption. Make sure that required reagents, materials and devices are prepared ready at the appropriate time. Allow all reagents and specimens to reach room temperature (18-25 °C) and gently swirl each vial of liquid reagent and sample before use. Mix reagents without foaming.
3. Avoid contamination of reagents, pipettes and wells/tubes. Use new disposable plastic pipette tips for each component and specimen. Do not interchange caps. Always cap not used vials. Do not reuse wells/tubes or reagents.
4. It is advised to determine samples in duplicate to be able to identify potential pipetting errors.
5. Use a pipetting scheme to verify an appropriate plate layout.
6. Incubation time affects results. All wells should be handled in the same order and time sequences. It is recommended to use an 8-channel Micropipettor for pipetting of solutions in all wells.
7. Microtiter plate washing is important. Improperly washed wells will give erroneous results. It is recommended to use a multichannel pipette or an automatic microtiter plate washing system. Do not allow the wells to dry between incubations. Do not scratch coated wells during rinsing and aspiration. Rinse and fill all reagents with care. While rinsing, check that all wells are filled precisely with Wash Buffer, and that there are no residues in the wells.

8. Humidity affects the coated wells/tubes. Do not open the pouch until it reaches room temperature. Unused wells/tubes should be returned immediately to the resealed pouch including the desiccant.

## 10. PRE-TEST SETUP INSTRUCTIONS


### 10.1. Preparation of concentrated components

	The contents of the kit for 96 determinations can be divided into 3 separate runs. The volumes stated below are for one run with 4 strips (32 determinations).					
Dilute / dissolve	Component	Diluent		Relation	Storage	Stability
15 mL	WASHBUF CONG	285 mL	bidist. water	1:20	2-8°C	1 month

### 10.2. Dilution of Samples

Sample	to be diluted	with	Relation	Remarks
Serum, Plasma	no			Avoid direct sunlight.
Urine	generally	ASSAYBUF	1:101	e.g. 10 µL + 1000 µL Avoid direct sunlight.

Samples containing concentrations higher than the highest standard have to be diluted further.

	Samples from patients treated with ATG (anti-T lymphocyte globulin from rabbit) after transplantation will cause erroneous high results. This effect can be avoided by a pre-incubation of the samples: Pipette 100 µL of serum into a Sarstedt or glass tube and add 200 µL of Assay Buffer. Close tubes (use pierced stopper for glass tubes) and incubate for 10 min in a waterbath at 95-100 °C. Vortex and withdraw 10 µL of the gel for the assay. Results have to be multiplied 3-fold.
--	---

## 11. TEST PROCEDURE

This enzyme immunoassay is evaluated for the manual use and especially for the automated use with the DadeBehring BEP2000 ELISA processor for the determination of neopterin in serum and plasma. Therefore the manual contains two different working procedures. The usage of this assay with other automated systems is possible. However in this case please contact IBL for further advices.

### 11.1. MANUAL PROCEDURE

1.	Pipette <b>20 µL</b> of each <b>Standard, Control, serum, plasma and diluted urine sample</b> into the respective wells of the Microtiter Plate.
2.	Pipette <b>100 µL Enzyme Conjugate</b> into each well.
3.	Pipette <b>50 µL of Neopterin Antiserum</b> into each well.
4.	Cover plate with <u>black</u> adhesive foil. <b>Incubate 90 min</b> at <b>RT (18-25 °C)</b> on an orbital shaker (500 rpm) in the dark.
5.	Remove adhesive foil. Discard incubation solution. Wash plate <b>4 x 300 µL</b> with diluted <b>Wash Buffer</b> . Remove excess solution by tapping the inverted plate on a paper towel.
6.	For adding of Substrate and Stop Solution use, if available, an 8-channel Micropipettor. Pipetting should be carried out in the same time intervals for Substrate and Stop Solution. Use positive displacement and avoid formation of air bubbles.
7.	Pipette <b>150 µL of TMB Substrate Solution</b> into each well.
8.	<b>Incubate 10 min</b> at <b>RT (18-25 °C)</b> .
9.	Stop the substrate reaction by adding <b>150 µL of TMB Stop Solution</b> into each well. Briefly mix contents by gently shaking the plate.
10.	<b>Measure</b> optical density with a photometer at <b>450 nm</b> (Reference-wavelength: 600-650 nm) within <b>15 min</b> .

## 11.2. AUTOMATED PROCEDURE

In the following chapter is described the procedure for a typical ELISA processor using BEP 2000 from Dade Behring as an example. IBL International provides also protocols for other commercially available devices e.g. Triturus from Grifols, DSX from Dynex, DS2 from Dynex, Tecan Genesis RSP, BEP3 from Dade Behring, Gemini from Stratec etc. Please contact us if you want to automatize your ELISA. Our application specialists are glad to assist you.

### Procedure for BEP2000 (Dade Behring) for serum and plasma

For valid runs on the Behring ELISA Processor BEP2000 only use the program file and reagent data base that is recommended by IBL. These files can be ordered by IBL International easily.

1.	Aspirate <b>110 µL Enzyme Conjugate</b> in one reagent tip (300 µL), and than aspirate additionally to that volume <b>20 µL</b> of each <b>Standard, Control or Sample in the same tip</b> .
2.	Pipette <b>120 µL</b> of that mixture ( <b>of Standard, Control or Sample with Enzyme Conjugate</b> ) in the respective wells of the microtiter plate.
3.	Pipette <b>50 µL</b> of <b>Antiserum</b> into each well.
4.	<b>Incubate 90 ± 5 min</b> at RT ( <b>18-25 °C</b> ) on an orbital shaker (frequency of 10 Hz; with an amplitude of 4 mm) in the dark.
5.	Aspirate supernatant. Wash plate <b>6 x</b> with <b>300 µL</b> diluted <b>Wash Buffer</b> .
6.	Pipette <b>150 µL</b> of <b>TMB Substrate Solution</b> into each well.
7.	<b>Incubate 10 ± 1 min</b> at RT ( <b>18-25 °C</b> ).
8.	Pipette <b>150 µL</b> of <b>TMB Stop Solution</b> into each well.
9.	<b>Measure</b> optical density with a photometer at <b>450 nm</b> (Reference-wavelength: 600-650 nm) within <b>15 min</b> .

## 12. QUALITY CONTROL

The test results are only valid if the test has been performed following the instructions. Moreover the user must strictly adhere to the rules of GLP (Good Laboratory Practice) or comparable standards/laws. User and/or laboratory must have a validated system to get diagnosis according to GLP. All kit controls must be found within the acceptable ranges as stated on the labels and the QC certificate. If the criteria are not met, the run is not valid and should be repeated. Each laboratory should use known samples as further controls. It is recommended to participate at appropriate quality assessment trials.

In case of any deviation the following technical issues should be proven: Expiration dates of (prepared) reagents, storage conditions, pipettes, devices, incubation conditions and washing methods.

## 13. CALCULATION OF RESULTS

The obtained OD of the standards (y-axis, linear) are plotted against their concentration (x-axis, logarithmic) either on semi-logarithmic graph paper or using an automated method. A good fit is provided with cubic spline, 4 Parameter Logistics or Logit-Log.

For the calculation of the standard curve, apply each signal of the standards (one obvious outlier of duplicates might be omitted and the more plausible single value might be used).

The concentration of the samples can be read directly from the standard curve.

Due to the dilution of urine samples the urine values obtained have to be multiplied by the factor 101.

Samples showing concentrations above the highest standard have to be diluted as described in PRE-TEST SETUP INSTRUCTIONS and reassayed.

### Conversion:

Based on the molecular weight of Neopterin (MW: 253.2 g/mol) and Creatinine (MW: 113.1 g/mol) a calculation in different units can be made as follows:

Serum/Plasma:

Neopterin	$(\text{nmol/L}) \times 0.253 = (\text{ng/mL})$
	$(\text{ng/mL}) / 0.253 = (\text{nmol/L})$

**Urine:**

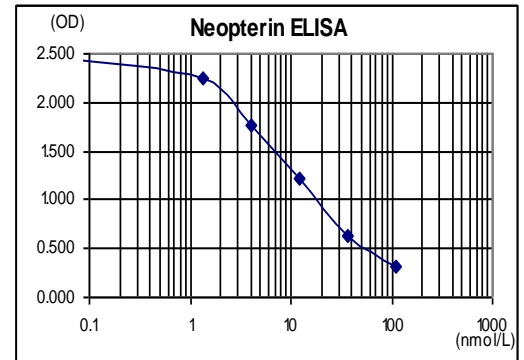
Usually neopterin in urine is correlated to creatinine (which has to be analyzed by separate method) and expressed in neopterin to creatinine - ratio (UNCR) in  $\mu\text{mol}$  neopterin/mol creatinine:

Creatinine	$(\text{mg/dL}) \times 88.4 = (\mu\text{mol/L})$
	$(\mu\text{mol/L}) / 1000 = (\text{mmol/L})$
	$(\text{mmol/L}) / 1000 = (\text{mol/L})$
Neopterin	$(\text{nmol/L}) / 1000 = (\mu\text{mol/L})$

**Typical Calibration Curve**

(Example. Do not use for calculation!)

Standard	Neopterin (nmol/L)	OD <sub>Mean</sub>	OD/OD <sub>max</sub>
A	0.00	2.449	100
B	1.35	2.238	91
C	4.00	1.772	72
D	12.0	1.209	49
E	37.0	0.634	26
F	111	0.325	13

**14. INTERPRETATION OF RESULTS**

Neopterin (Serum)	Interpretation
< 10 nmol/L	normal
> 10 nmol/L	elevated

The results themselves should not be the only reason for any therapeutical consequences. They have to be correlated to other clinical observations and diagnostic tests.

**15. EXPECTED VALUES**

Apparently healthy subjects show the following values:

Serum		Serum			(Neopterin Biochemistry – Methods - Clinical Application; H. Wachter et al. (1992), Walter de Gruyter, Berlin - New York)	
nmol/L	ng/mL	Age	Sex	Neopterin nmol/L		
< 10	< 2.5			Mean		upper limit
		0-18	♂, ♀	6.78		13.5
		19-75	♂, ♀	5.34	8.7	
		> 75	♂, ♀	9.67	19.0	

Urine				(Neopterin Biochemistry – Methods - Clinical Application; H. Wachter et al. (1992), Walter de Gruyter, Berlin - New York)
Age	Sex	$\mu\text{mol}$ Neopterin/mol Creatinine		
		Mean	upper limit	
1-4	♂, ♀	267	432	
4-7	♂, ♀	226	405	
7-12	♂, ♀	181	374	
12-15	♂, ♀	171	343	
15-18	♂, ♀	144	320	
	♂	123	195	
18-25	♀	128	208	
	♂	101	182	
26-35	♀	124	209	
	♂	109	176	
36-45	♀	140	239	
	♂	105	197	
46-55	♀	147	229	
	♂	119	218	
56-65	♀	156	249	
	♂	133	229	
>65	♀	151	251	

It is recommended that each laboratory establishes its own range of normal values.

## 16. LIMITATIONS OF THE PROCEDURE

Specimen collection and storage have a significant effect on the test results. See SPECIMEN COLLECTION AND STORAGE for details.

For cross-reactivities, see PERFORMANCE.

The following blood components do not have a significant effect (+/- 20 % of expected) on the test results up to the below stated concentrations:	Hemoglobin	5.0 mg/mL
	Bilirubin	2.5 mg/mL
	Triglyceride	45.5 mg/mL

**Do not use samples containing sodium azide** since these samples lead to erroneous high results.

Samples from patients who were treated with ATG (anti-T lymphocyte globulin from rabbit) after transplantation will cause erroneous high results. This effect can be avoided by a pre-incubation of the samples as described in PRE-TEST SETUP INSTRUCTIONS.

## 17. PERFORMANCE











<b>Analytical Specificity (Cross-reactivity)</b>	Substance		Cross Reactivity (%)	Cross-reactivity of other substances tested < 0.05 %
	7,8-Dihydro-Neopterin		2.0	
	5,6,7,8-Tetrahydro-Neopterin		< 0.44	
	D-Monapterin		< 0.17	
	L-Monapterin		< 0.03	
	7,8-Dihydro-L-Biopterin		< 0.01	
<b>Analytical Sensitivity (Limit of Detection)</b>	0.7 nmol/L	Mean signal (Zero-Standard) - 2SD		
<b>Precision</b>		Range (nmol/L)	CV (%)	
Intra-Assay	Serum	3.1 - 43	4.3 – 11.7	
	Urine	932 - 5112	5.3 – 11.2	
Inter-Assay	Serum	4.67 – 29.98	8.8 – 13.8	
	Urine	2616 - 4419	9.3 – 14.4	
<b>Linearity</b>		Range (nmol/L)	Range (%)	Serial dilution up to
	Serum	1.8 – 51.5	91 – 114	1:16
	Urine	234 - 3622	87 – 120	1:8
<b>Recovery</b>		Mean (%)	Range (%)	% Recovery after spiking
	Serum	99	81 – 116	
	Urine	94	84 – 117	
<b>Method Comparison versus HPLC</b>	Serum	IBL-Assay = 1.18 x HPLC + 0.44		r = 0.92; n = 111
	Urine	IBL-Assay = 1.17 x HPLC – 13.52		r = 0.99; n = 27



**18. PRODUCT LITERATURE REFERENCES**

1. Wachter H, Fuchs D, Hausen A, Reibnegger G, Weiss G, Werner ER, Werner-Felmayer G. Neopterin: Biochemistry - Methods - Clinical Application. Walter de Gruyter Berlin, New York, (1992)
2. Westermann J, Thiemann F, Gerstner L, Tatzber F, Kozák I, Bertsch T, Krüger C. Evaluation of a New Simple and Rapid Enzyme-Linked Immunosorbent Assay Kit for Neopterin Determination. *Clin Chem Lab Med*, 38 (4): 345-353 (2000)
3. X Garcia-Moll, D Cole, E Zouridakis, JC Kaski. Increased serum Neopterin: a marker of coronary artery disease activity in woman. *Heart* 83:346-350 (2000)
4. Smith D, Zouridakis, E, Mariani M, Fredericks S, Cole D, Kaski J. Neopterin levels in patients with coronary artery disease are independent of Chlamydia pneumoniae seropositivity. *Am Heart J*, 146 (1): 69-74 (2003)
5. B. Inci Fisenk, Durdal US, Osman I. Ozcebe & Gulsen Hascelik. The value of increased Neopterin levels in reducing transfusion-transmitted virus infections: Detection of a donation from a HbsAg positive chronic carrier by screening of neopterin in Turkish blood donors. *Scandinavian Journal of Infectious disease*, 37:599-604 (2005)
6. Michaela Bayer, Sven Schmitz, Jürgen Westermann, Frank Thiemann, Ralf Edelmann, Claudia Szakacs, Gerhardt Lanzer, Jens Blecken. Evaluation of a New-Linked Immunosorbent Assay for the Determination of Neopterin. *Clin Lab*. 51 (2005)
7. R. Weimer, C. Süsal, S. Yildiz, A. Staak, S. Pelzl, F. Renner, H. Dietrich, V. Daniel, S. Kamali-Ernst, W. Padberg, G. Opelz. Post-Transplant sCD30 and Neopterin as Predictors of Chronic Allograft Nephropathy: Impact of Different Immunosuppressive Regimes. *American Journal of Transplantation* (2006)
8. Cangel P.Y. Chan, Junet W.Y. Choi, Kai-Yuan Cao, Ming Wang, Yang Gao, Duan-Hua Zhou, Biao Di, Hui-Fang Xu, Man-Fai Leung, Andreas Bergmann, Matthias Lehmann, Yong-Mei Nie, George W.H. Cautherley, Dietmar Fuchs, Reinhard Renneberg, Bo-Jian Zheng. Detection of serum neopterin for early assessment of dengue virus infection. *Journal of Infection* (2006)
9. Douglas T. Johnston, Marios Gagos, Nicolas Raio, Louis Ragolia, David Shenouda, Mark A. Davis-Lorton, Joshua R. De Leon. Alterations in serum neopterin correlate with thrombolysis in myocardial infarction risk scores in acute coronary syndromes. *Coronary artery disease* 2006, 17:511-516
10. SP Giese, EM Crone, EA Flavall, Z Amit. Potential to inhibit growth of atherosclerotic plaque development through modulation of macrophages neopterin/ 7,8-dihydroneopterin synthesis. *British Journal of Pharmacology* (2007)
11. Kausik K. Ray, David A. Morrow, Marc S. Sabatine, Amy Shui, Nader Rifai, Christopher P. Cannon, Eugene Braunwald. *Circulation* 2007; 115; 3071:3078

# Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di evaluazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED.  Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben.  Voir MATERIEL FOURNI pour les symbôles des composants du kit.  Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS.  Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS.  Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT.  Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

**COMPLAINTS:** Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

**WARRANTY:** The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

**LIMITATION OF LIABILITY:** IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

	<b>IBL International GmbH</b>	Tel.: + 49 (0) 40 532891 -0 Fax: -11
	Flughafenstr. 52A, 22335 Hamburg, Germany	E-MAIL: IBL@IBL-International.com
		WEB: <a href="http://www.IBL-International.com">http://www.IBL-International.com</a>